

## Effects of Seeding Procedures and Water Quality on Recovery of *Cryptosporidium* Oocysts from Stream Water by Using U.S. Environmental Protection Agency Method 1623

Donna S. Francy,<sup>1\*</sup> Otto D. Simmons III,<sup>2</sup> Michael W. Ware,<sup>3</sup> Emma J. Granger,<sup>1</sup>  
Mark D. Sobsey,<sup>2</sup> and Frank W. Schaefer III<sup>3</sup>

U.S. Geological Survey, Columbus, Ohio 43229<sup>1</sup>; School of Public Health, University of North Carolina—Chapel Hill, Chapel Hill, North Carolina 27599-7400<sup>2</sup>; and U.S. Environmental Protection Agency, Cincinnati, Ohio 45268<sup>3</sup>

Received 2 February 2004/Accepted 31 March 2004

U.S. Environmental Protection Agency method 1623 is widely used to monitor source waters and drinking water supplies for *Cryptosporidium* oocysts. Matrix spikes, used to determine the effect of the environmental matrix on the method's recovery efficiency for the target organism, require the collection and analysis of two environmental samples, one for analysis of endemic oocysts and the other for analysis of recovery efficiency. A new product, ColorSeed, enables the analyst to determine recovery efficiency by using modified seeded oocysts that can be differentiated from endemic organisms in a single sample. Twenty-nine stream water samples and one untreated effluent sample from a cattle feedlot were collected in triplicate to compare modified seeding procedures to conventional seeding procedures that use viable, unmodified oocysts. Significant negative correlations were found between the average oocyst recovery and turbidity or suspended sediment; this was especially apparent in samples with turbidities greater than 100 nephelometric turbidity units and suspended sediment concentrations greater than 100 mg/liter. *Cryptosporidium* oocysts were found in 16.7% of the unseeded environmental samples, and concentrations, adjusted for recoveries, ranged from 4 to 80 oocysts per 10 liters. Determining recovery efficiency also provided data to calculate detection limits; these ranged from <2 to <215 oocysts per 10 liters. Recoveries of oocysts ranged from 2.0 to 61% for viable oocysts and from 3.0 to 59% for modified oocysts. The recoveries between the two seeding procedures were highly correlated ( $r = 0.802$ ) and were not significantly different. Recoveries by using modified oocysts, therefore, were comparable to recoveries by using conventional seeding procedures.

To improve monitoring for *Cryptosporidium* oocysts in water, the U.S. Environmental Protection Agency (USEPA) developed methods 1622 (30) and 1623 (31), which consist of filtration, concentration, immunomagnetic separation (IMS), fluorescent antibody and 4',6'-diamidino-2-phenylindole (DAPI) counter staining, and microscopic detection and enumeration. Method 1622 detects and enumerates only *Cryptosporidium* in water samples; method 1623 detects and enumerates *Cryptosporidium* oocysts and *Giardia* cysts in water samples and incorporates improvements over the previous method. Both are performance-based methods, allowing components to be replaced by other more efficient or effective components, provided the substitutions meet required quality control acceptance criteria.

Recoveries of oocysts from environmental water samples with method 1622 or 1623, however, have been found to be highly variable (15, 26, 32). Because of variable recoveries, matrix spikes are routinely analyzed to determine the effect of the environmental matrix on the method's recovery efficiency for the target organisms. In conventional seeding procedures for these methods, two samples are analyzed, one of which is seeded with known numbers of viable organisms (matrix spike) and the other of which is unseeded. A potential modification

for method 1623 is to use an alternative seeding procedure, ColorSeed, which enables the analyst to determine the percent recovery and number of environmental oocysts in one water sample. In this product, organisms are modified to incorporate a fluorochrome that is used to distinguish seeded organisms from unmodified organisms that may be present in the environmental sample. Modified organisms are gamma irradiated to increase stability, whereas conventional seeding procedures use viable organisms. Gamma irradiation also inactivates the oocysts, decreasing the health risk for the laboratory analyst compared to the risk of using viable organisms. If the modified seeding procedure is found to yield equivalent percent recoveries to that of the conventional seeding procedure, sampling and analytical time would be significantly reduced for processing environmental water samples.

In this study, 30 stream water samples were collected from 20 sites throughout the United States to compare the recovery efficiencies of *Cryptosporidium* oocysts by method 1623 with modified and conventional seeding procedures. For each sample, one unseeded and two seeded subsamples were analyzed. The collection and processing of these samples afforded the opportunity to address other issues regarding the use of method 1623 for monitoring environmental waters. These issues included determining whether water quality factors affected recoveries of oocysts by method 1623 and whether fecal indicators (*Escherichia coli*, *Clostridium perfringens*, and somatic and F-specific coliphage) could be used as surrogates for the presence of *Cryptosporidium* in stream waters.

\* Corresponding author. Mailing address: U.S. Geological Survey, Water Resources Discipline, 6480 Doubletree Ave., Columbus, OH 43229. Phone: (614) 430-7769. Fax: (614) 430-7777. E-mail: dsfrancy@usgs.gov.

Several studies have attempted to identify water quality properties and constituents that affect recoveries of oocysts by using method 1622 or 1623. Many investigators found that turbidity was related to recoveries of oocysts (4, 5, 7, 15, 26). The efficiency of the IMS technique was shown to decrease when the adjusted pH deviated from 7.0 (16) or when dissolved iron concentrations were greater than 4 mg/liter (38). In contrast, in the Information Collection Rule Supplemental Survey (ICRSS), wherein 430 samples were collected from 87 source waters, all measured water quality properties, including turbidity, were found to be unrelated or weakly related to recoveries of oocysts (32).

In addition to improving the performance of method 1623, there is continued interest in identifying a microbiological surrogate for the presence of *Cryptosporidium* in water. Microbiological surrogates investigated in previous studies have included *E. coli*, *C. perfringens*, fecal coliforms, total coliforms, and somatic and F-specific coliphage. Previous surface water studies have shown significant relations between detection and enumeration of oocysts and some of these fecal indicators (2, 18, 19, 20, 32). In contrast, other researchers found no significant relations between indicator organisms and *Cryptosporidium* in wastewater (3), in drainage canals (W. E. McElroy, S. Pillai, E. Cabello, and S. Hernandez, Abstr. 101st Gen. Meet. Am. Soc. Microbiol. Abstr. Q-230, p. 629-630, 2001), or in surface waters (21, 22, 23).

In this study, we tested the use of the modified seeding procedure and found it to be an acceptable alternative seeding procedure for the detection of *Cryptosporidium* by using method 1623. We demonstrated the importance of including appropriate quality control samples in any monitoring program. The relations between recoveries of *Cryptosporidium* and water quality properties were examined. Of the water quality properties tested, a negative relation was found between recovery and turbidity or suspended-sediment concentrations. Because *Cryptosporidium* oocysts were found in a small percentage of the 30 samples collected, we were not able to examine the relation between the detection of *Cryptosporidium* and concentrations of fecal indicators.

#### MATERIALS AND METHODS

**Site selection and sample collection.** Twenty sites were selected to include broad geographic coverage of the United States (Table 1). If two sites were in the same state, they are labeled as state 1 and state 2 in Table 1. The sites are part of the U.S. Geological Survey (USGS) National Water Quality Assessment Program, a national water quality program that focuses on "study units" that represent major hydrologic systems of the United States (13). A major criterion for site selection was to include sites with high probabilities of detecting target organisms, for example, sites potentially receiving human sewage or livestock inputs.

The site information in Table 1 shows that samples were collected from sites with a range of land use practices, drainage areas, and population densities. Thirty samples were collected between March 2002 and June 2003, 29 of which were collected from streams. The exception was the Colorado 1 effluent sample, which was collected from a drainage ditch on a cattle feedlot. Instantaneous stream flows were estimated at the time of sampling (Table 1) from a stage-stream flow relation developed for each site (14). Samples were placed into three categories based on historical stream flow data: (i) high (stream flow was greater than 90% of all measured stream flows at that site), (ii) elevated (stream flow was between 50 and 90% of all measured stream flows at that site), and (iii) base (stream flow was less than 50% of all measured stream flows at that site). For 10 stream water sites, samples were collected twice; eight of these samples were collected during base flow and elevated or high flow. These sites were expected

to receive fecal contamination during different flow conditions. The two Washington 1 samples were collected at base flow during the irrigation season and the two Alabama 2 samples were collected at elevated flow. The "a" and "b" designations for these samples in Table 1 indicate two samples collected at the same site with stream flows in the same category. For the 10 sites in which only one sample was collected, based on the sampler's experience, a base-, elevated-, or high-flow sample was collected to sample when fecal contamination was expected to be greatest.

For *Cryptosporidium* analyses, three 10-liter sterile, disposable, collapsible cubitainers (Eagle Picher Technologies, Miami, Okla.) were filled with water collected from several vertical sampling intervals in the stream cross section. Samples were similarly collected in a 3-liter sterile sample bottle and analyzed for *C. perfringens*, coliphage, *E. coli*, and turbidity. Specific conductance, temperature, dissolved oxygen, and pH were measured in the stream with a four-parameter water quality meter and USGS protocols (37). Alkalinity was determined by field crews using the incremental titration technique (37). Samples for water quality constituents were collected by using USGS protocols (24). Human population densities for each site were obtained from the U.S. Bureau of the Census (27) and were calculated from countywide coverages by applying densities as a percentage of the county in the watershed.

***Cryptosporidium parvum* oocysts.** Viable *Cryptosporidium parvum* (Harley Moon strain) oocysts used for the conventional seeding procedure were obtained from C. Sterling, University of Arizona, and were propagated in dexamethasone-immunosuppressed C57BL female mice at the USEPA facility in Cincinnati, Ohio (6). The oocysts were purified with sieving, step sucrose gradients, and cesium chloride purification (1). These highly purified oocysts were suspended in reagent-grade water containing 100 U of penicillin and 100 µg of streptomycin/ml, stored at 4°C, and used within 5 weeks of purification.

A FACS VantageSE (Beckton Dickinson, Palo Alto, Calif.) flow cytometry system equipped with CloneCyt software was used for the preparation of all viable oocyst seeding preparations. Isoton II (Coulter Corp., Hiialeah, Fla.) was used as the sheath fluid during cell sorting. A gate was drawn around the unstained oocysts by using forward scatter (FSC) and side scatter (SSC), with both FSC and SSC measured linearly with a gain of 1, an SSC detector set at 399 V, and an FSC threshold set at 32 V. For each seeding suspension, 100 oocysts were sorted into a 1.5-ml microcentrifuge tube containing 1 ml of aqueous 0.01% Tween 20. In addition to the tubes used for seeding, additional tubes were similarly prepared for microscopic verification and trip controls that are further described below. The oocysts were sent on ice by overnight courier to the USGS Ohio District Microbiology Laboratory and were used within 1 week of cell sorting.

The modified oocysts used during this study came from the manufacturer (Biotechnology Frontiers, North Ryde, New South Wales, Australia) in sealed vials containing approximately 100 *Cryptosporidium parvum* oocysts. These oocysts were sorted by the manufacturer using flow cytometry after having been gamma irradiated and embedded with a fluorochrome by using a proprietary method. Each vial arrived with a certificate of analysis that documented the mean oocyst concentration and standard deviation in each vial.

**Filtration, elution, and concentration of *Cryptosporidium* from water samples.** The three replicate 10-liter water samples to be analyzed for *Cryptosporidium* oocysts were sent to the USGS Ohio District Microbiology Laboratory within 48 h of sample collection. At the laboratory, the samples were seeded (when applicable), filtered, eluted, and concentrated by use of method 1623 with some modifications to obtain (i) a regular sample (no seed), (ii) a sample seeded with modified oocysts, and (iii) a sample seeded with viable oocysts by the conventional seeding method.

Samples were processed by using a Hemoflow F80A ultrafilter, a polysulfone hollow-fiber single-use unit with an 80,000 molecular weight cutoff (Fresenius USA, Lexington, Mass.) (25). A peristaltic pump (Geotech Environmental Equipment, Inc., Denver, Colo.) was used to recirculate the water within a closed ultrafiltration system at a pressure of 20 to 25 lb/in<sup>2</sup>. When the volume of the sample was reduced to the hold-up volume of the ultrafilter system, oocysts were eluted from the ultrafilter by recirculating 250 ml of eluting solution (100 mM phosphate-buffered saline with 1% Laureth 12) at low pressure (5 to 10 lb/in<sup>2</sup>) through the system. The eluate was collected in a 250-ml centrifuge tube along with any additional liquid that was purged from the ultrafilter with air pressure (less than 25 lb/in<sup>2</sup>). The oocysts were further concentrated by centrifugation at 1,500 × g and 4°C for 15 min in an International Equipment Company (Needham Heights, Mass.) model IEC PR-7000 M centrifuge with a swinging bucket rotor. The supernatant was aspirated from the concentrated sample to the 5-ml mark on the centrifuge tube or to 3 ml above the pellet, whichever volume was greater. The pellet was transferred to a 15-ml centrifuge tube that was pretreated with SigmaCote (Sigma, St. Louis, Mo.), and the 250-ml centrifuge tube was

TABLE 1. Characteristics of stream water sampling sites, 2002 to 2003

Stream water site <sup>a</sup>	Stream flow condition <sup>b</sup>	Land use	Potential sources of fecal contamination <sup>c</sup>	Drainage area (square miles)	Population density (people/square mile)	Stream flow at time of sampling (cubic feet/s) <sup>f</sup>
Alabama 1	Elevated	Mixed (agricultural and forest)	Feedlots and septic systems	374	33,000	163
Alabama 2a <sup>d</sup>	Elevated	Agricultural	Free-range cattle and septic systems	29	2,100	36
Alabama 2b <sup>d</sup>	Elevated	Agricultural	Free-range cattle and septic systems	29	2,100	44
Colorado 1 <sup>e</sup>	Effluent	Agricultural	CAFOs, applied manure, wildlife, and septic systems	567	5.9	NA
Colorado 2	Elevated	Mixed (forest, rangeland, agricultural, and urban)	WWTPs, CAFOs, applied manure, and wildlife	9,598	300	628
Georgia 1	Base	Mixed (urban, forest, and agricultural)	Large urban WWTP and combined-sewer overflows	2,060	690	1,140
Georgia 1	High	Mixed (urban, forest, and agricultural)	Large urban WWTP and combined-sewer overflows	2,060	690	8,400
Georgia 2	High	Urban residential	Septic systems	29	2,100	183
Indiana	Elevated	Agricultural	Cows, septic systems, and WWTPs	610	61	142
Iowa <sup>d</sup>	Base	Agricultural	Hog CAFOs and manure	230	16	48
Iowa <sup>d</sup>	High	Agricultural	Hog CAFOs and manure	230	16	967
Louisiana <sup>d</sup>	Base	Urban residential and commercial	WWTP and combined-sewer overflows	15	3,000	2.2
Louisiana <sup>d</sup>	Elevated	Urban residential and commercial	WWTP and combined-sewer overflows	15	3,000	20
Nebraska	High	Agricultural	Feedlots and septic systems	369	11	153
Nebraska	Base	Agricultural	Feedlots and septic systems	369	11	23
Ohio	Elevated	Agricultural	Cows and WWTPs	310	130	209
Ohio	High	Agricultural	Cows and WWTPs	310	130	668
South Carolina 1	Base	Agricultural	CAFOs	23	210	7.4
South Carolina 1	Elevated	Agricultural	CAFOs	23	210	15
South Carolina 2	Elevated	Urban	WWTPs, street runoff, and raw sewage	60	1,800	65
Texas	Elevated	Mixed (urban and agricultural)	WWTPs, street runoff, and raw sewage	6,278	410	4,030
Texas	Base	Mixed (urban and agricultural)	WWTPs, street runoff, and raw sewage	6,278	410	340
Virginia 1	Base	Urban residential and commercial	Wildlife, recreation, and WWTPs	24	110,000	2.2
Virginia 2 <sup>d</sup>	Elevated	Agricultural	Feedlots and septic systems	14	110	14
Washington 1a <sup>d</sup>	Base	Agricultural	Dairy CAFOs and applied manure	62	49	53
Washington 1b <sup>d</sup>	Base	Agricultural	Dairy CAFOs and applied manure	62	49	38
Washington 2	High	Urban residential and commercial	WWTPs, street runoff, and wildlife	12	5,600	31
Wisconsin 1	High	Agricultural	Septic systems, dairy farms, and WWTPs	96	85	155
Wisconsin 2	Base	Mixed (urban and agricultural)	Septic systems, feedlots, applied manure, and WWTPs	696	520	88
Wisconsin 2	High	Mixed (urban and agricultural)	Septic systems, feedlots, applied manure, and WWTPs	696	520	993

<sup>a</sup> If two sites were in the same state, they are labeled as state 1 and state 2. If two samples were collected at the same site and streamflow category, they are labeled as "a" and "b."

<sup>b</sup> High, streamflow was greater than 90% of all measured streamflows at that site; elevated, streamflow was between 50 and 90% of all measured streamflows at that site; base, streamflow was less than 50% of all measured streamflows at that site.

<sup>c</sup> CAFO, concentrated animal feeding operation; WWTP, wastewater treatment plant.

<sup>d</sup> Ten-year period of record data was not available, so streamflow categories were estimated.

<sup>e</sup> Sample was collected from a drainage ditch on a cattle feedlot.

<sup>f</sup> NA, not applicable.

rinsed twice with sterile reagent water. The pellet was sent to the University of North Carolina (UNC) laboratory at Chapel Hill, N.C., on ice by overnight courier for further processing and analysis.

**IMS and staining of *Cryptosporidium* oocysts.** At the UNC laboratory, anti-*Cryptosporidium* IMS kits (DynaL Inc., Lake Success, N.Y.) were used to separate oocysts within the samples from other extraneous particulate matter by using the protocol described in method 1623 with one major modification: the acid-based dissociation step was replaced with heat dissociation (35). For heat dissociation, the sample was heated at 80°C for 10 min in a heating block. Only one IMS purification was performed for each sample. Following IMS, samples were transferred to well slides (Meridian Diagnostics, Cincinnati, Ohio) and dried in a desiccating chamber for approximately 2 h or overnight. The slides were fixed

with absolute methanol and stained with a fluorescein-labeled direct antibody kit (Crypt-a-Glo, Waterborne, Inc., New Orleans, La.) and counterstained with DAPI (0.02 mg/ml; Sigma). After the slides were stained, a glycerol-1,4-diazabicyclo-[2.2.2] octane (DABCO) mounting medium (Sigma) was added to each well and a coverslip was applied. Slides were stored in the desiccator in the dark until they were microscopically examined, which was done within 72 h of staining.

**Quality control samples for *Cryptosporidium* analysis.** Quality control samples to demonstrate method proficiency included initial precision and recovery (IPR) and ongoing precision and recovery (OPR) experiments, method blanks, IMS controls, and stain controls. Four IPRs and three OPRs were performed by processing three 10-liter volumes of reagent-grade water, one unseeded (method blank) and two seeded with 100 *Cryptosporidium* oocysts (either viable or mod-

TABLE 2. Quality control samples for *Cryptosporidium* analysis with method 1623

Sample	Date (mo/day/yr)	% Recovery (RSD) with <sup>a</sup> :		Method blank	% IMS controls (RSD)	
		Viable oocysts	ColorSeed		Positive	Negative
IPR samples						
1	12/04/2001	45	34	0	70	0
2	12/11/2001	47	40	0	64	0
3	01/08/2002	41	55	0	69	0
4	01/29/2002	23	31	0	66	0
Avg		39 (28) <sup>b</sup>	40 (27) <sup>b</sup>		67 (4)	
OPR samples						
1	07/08/2002	55	51	0	82	0
2	12/09/2002	47	41	0	76	0
3	06/10/2003	57	52	0	50 <sup>d</sup>	0
Avg		53 (10) <sup>c</sup>	48 (13) <sup>c</sup>	0	79 (5)	0

<sup>a</sup> RSD is the relative standard deviation.

<sup>b</sup> Acceptable range for recovery is 24 to 100%; acceptable maximum RSD is 55%.

<sup>c</sup> Acceptable range for recovery is 11 to 100%.

<sup>d</sup> Slide was dropped and cracked, so counts are underestimated; this value was not used in average and statistical analyses.

ified) as described above. Positive and negative IMS and stain controls were included with each set of samples. The negative IMS control was prepared by replacing the sample with reagent water at the beginning of the IMS procedure. The positive IMS control was prepared by replacing the sample with 1 ml of viable flow-counted oocysts brought to volume with reagent water. IMS controls were then processed in the same manner as the regular environmental water samples. The IMS controls were included to demonstrate the recovery efficiency of the IMS part of the method. Stain controls were processed according to the manufacturer's instructions to ensure reliable oocyst staining during each set of experiments.

Microscopic counts analyzed with each set of samples were used to verify concentrations of oocyst seeds (confirmation controls) or to monitor the effects of travel and time on oocysts (trip controls). For all microscopic counts, a test tube containing oocysts prepared for seeding was shaken by hand for 30 s, the sample was transferred by pipette and filtered through a 0.8- $\mu$ m-porosity, 13-mm-diameter black polycarbonate filter, and the tube was rinsed with 1 ml of reagent water that was then filtered. The oocysts were stained with 100  $\mu$ l of 1 $\times$  Crypta-glo stain solution for 30 min. After the filter was transferred to a glass slide and mounted in DAPCO mounting medium, the oocysts were microscopically enumerated. In this manner, the following counts of viable oocysts prepared at USEPA were done: (i) initial counts at USEPA, (ii) confirmation controls shipped from USGS to UNC and counted at UNC, (iii) trip controls shipped from USGS to USEPA and counted at USEPA, and (iv) trip controls shipped from USGS to UNC to USEPA and counted at USEPA. For modified oocysts, confirmation controls were microscopically analyzed at the UNC laboratory.

**Analysis of water samples for microbiological indicators and water quality.** Water samples were analyzed for microbiological indicators and turbidity at the USGS Ohio laboratory within 24 h of sample collection. Samples for enumeration of *C. parvum* were analyzed by use of the mCP agar method (29) with the following modifications: samples were not heated to remove vegetative cells, holding times exceeded the recommended 8 h, and plates were incubated at 42°C instead of 44.5°C. For *C. parvum*, 30-, 10-, and 3-ml sample volumes were processed to obtain a countable dilution for each sample analyzed. Somatic and F-specific coliphage in 100-ml sample volumes were analyzed by using the single-agar layer method (33). Analyses of water samples for *E. coli* were done by using the mTEC membrane filtration method (28), and sample volumes of 100, 30, 10, 3, 1, and 0.3 ml were chosen to obtain plates within the ideal count range. Quality assurance and quality control procedures for microbiological indicators are described in detail at the USGS Ohio District Microbiology website (<http://oh.water.usgs.gov/micro/lab.html#qcm>).

Turbidity was measured by means of a Hach (Loveland, Colo.) model 2100P portable turbidimeter, and all turbidity measurements were made in duplicate. Water samples were also analyzed for concentrations of suspended sediment, nitrite plus nitrate, total phosphorus, silica, and iron at the USGS National Water Quality Laboratory in Lakewood, Colo., by USGS methods (8, 9, 10).

**Data analysis and statistical methods.** For environmental water samples that yielded pellet volumes greater than 0.5 ml, the entire sample volume was not examined. Percent recoveries (*REC*) were adjusted for the pellet volume and calculated as follows:

$$REC = \frac{(N - NSAMPLE)/CC}{0.5 \text{ ml}/PV} \times 100 \quad (1)$$

where *N* is the number of oocysts found in the seeded environmental sample, *NSAMPLE* is number of oocysts found in the unseeded environmental sample, *CC* is the certified oocyst count (100 for viable oocysts or certificate of analysis for modified oocysts, both sorted by flow cytometry), and *PV* is the pellet volume.

At the 10 sites where two samples were collected, the percent differences in recoveries between the two samples (*REC*<sub>1,2</sub>) were calculated as follows:

$$REC_{1,2} = \frac{ABS(REC_1 - REC_2)}{(REC_1 + REC_2)/2} \times 100 \quad (2)$$

where *ABS* is the absolute value, *REC*<sub>1</sub> is the percent recovery for sample 1, and *REC*<sub>2</sub> is percent recovery for sample 2.

Estimated oocysts in environmental samples per 10 liters, adjusted for average recoveries, were calculated as follows:

$$\text{oocysts}/10 \text{ liters} = \frac{10}{VE} \times \frac{100}{REC_{avg}} \times NSAMPLE \quad (3)$$

where *VE* is volume examined (liters), *REC*<sub>avg</sub> is average recovery of modified and viable oocysts, and *NSAMPLE* is number of oocysts found in the unseeded environmental sample. For samples in which no oocysts were found, the above equation was used with a value of 1 for *NSAMPLE*, and results were expressed in terms of "less than."

Because not all of the data were distributed normally, nonparametric statistical methods were used. The Wilcoxon signed-rank test was used to compare two groups of paired data. For comparing more than two groups of unpaired data, the nonparametric analysis of variance, the rank transform test, was used. If the analysis of variance showed significant differences among groups at  $\alpha = 0.05$ , the Tukey-Kramer multiple comparison test was used to determine which group's median ranks differed from each other (11).

## RESULTS

**Quality control samples.** The results of IPRs, OPRs, method blanks, and IMS controls are summarized in Table 2. Recoveries for three out of four IPRs were within acceptable limits for viable and modified oocysts, and the relative standard deviations were within the acceptable percentage, as described in

TABLE 3. Microscopic counts of viable and modified oocysts in confirmation and trip controls

Sample set	No. of viable oocysts				No. of modified oocysts
	Initial counts at USEPA (group A) <sup>a</sup>	Confirmation controls counted at UNC (group B) <sup>b</sup>	Trip controls from USGS to USEPA counted at USEPA (group C) <sup>c</sup>	Trip controls from USGS to UNC to USEPA counted at USEPA (group D)	Confirmation counts at UNC (group E)
1	97	94	94	97	80 <sup>d</sup>
2	98	91	97	94	89
3	95	88	98	93	97
4	98	101	99	97	92
5	93	97	98	92	96
6	94	88	94	92	93
7	97	92	92	94	89
8	96	53 <sup>c</sup>	90	88	51 <sup>c</sup>
9	94	90	ND	88	96
10	93	90	100	93	98
11	94	94	91	91	84
12	95	88	92	94	90
13	96	94	98	94	94
14	96	88	87	90	90
Avg	95.4	91.9	94.6	92.6	92.3
SD	1.7	4.0	4.0	2.8	4.1

<sup>a</sup> Each value is the mean of three counts done by the same analyst.

<sup>b</sup> Each value is the mean of two counts done by the same analyst.

<sup>c</sup> Slide did not stain well, so counts are underestimated; this value was not used in average and statistical analyses.

<sup>d</sup> Slide had air bubbles, so counts are underestimated; this value was not used in average and statistical analyses.

<sup>e</sup> ND, not determined.

method 1623. All OPRs for *Cryptosporidium* were within acceptable limits. Although viable oocyst recoveries were higher than modified oocyst recoveries in five out of seven IPR and OPR trials, a paired statistical comparison indicated no significant difference between these two groups. No oocysts were detected in any of the method blanks. Recoveries for the IMS positive controls ranged from 64 to 82% during IPR and OPR experiments.

Microscopic counts for five groups (A through E) of confirmation or trip controls are listed in Table 3. Microscopic counts were always less than certified flow cytometry counts. Certified counts for viable oocysts were 100 for all tubes. Certified counts for modified oocysts were 98 for sample sets 1 and 2 and 99 for the other sample sets. A different analyst counted the oocysts in groups B and E from groups A, C, and D, and different sources of oocysts were counted in groups B and E. Therefore, to determine whether viable oocysts degraded during shipping and handling, the results from microscopic counts of trip controls counted by the same analyst and obtained from the same source were examined by using statistical tests. After removal of outliers that were known to be biased low because of lab error, paired statistical tests between groups A, C, and D were examined. Statistical tests showed no significant difference between groups A and C ( $P = 0.394$ ) and groups C and D ( $P = 0.0743$ ). There was, however, a statistically significant difference between groups A and D ( $P = 0.0007$ ). This result indicates that degradation of viable oocysts occurred as the result of shipping and handling during four-legged trips (from USEPA to USGS to UNC to USEPA [group A to group D]) but not during three-legged trips (from USEPA to USGS to USEPA [group A to group C]).

**Recoveries of oocysts from stream water samples by using modified and conventional seeding procedures.** *Cryptosporidium* recoveries and associated sample-processing data from stream water samples seeded with viable and modified oocysts are shown in Table 4. The volumes of environmental water samples that were filtered ranged from 5.0 to 10.5 liters. The cubitainers used in this study can hold up to 10.5-liter volumes, but field crews often filled the containers to less than capacity, or water was lost during transport or processing. Because only up to 0.5 ml of concentrated pellet volume was examined by IMS, the volume examined was sometimes less than the volume filtered. For two samples, only about half of the volume was filtered because the filter clogged and filtration was no longer efficient; in these samples, the turbidities were 59 for the Georgia 1 high sample and 2,700 for the Nebraska high sample. Adjusted recoveries of oocysts ranged from 2.0 to 61% for viable oocysts and 3.0 to 59% for modified oocysts. IMS positive control recoveries were higher than adjusted recoveries, ranging from 58 to 87%.

Recoveries of viable oocysts are compared to recoveries of modified oocysts for each sample on a scatter plot (Fig. 1). The recoveries between the two seeding procedures were highly correlated ( $r = 0.802$ ), and the data were evenly scattered around the equal recovery line. Results from a paired two-way test showed that modified and viable oocyst recoveries were not significantly different ( $P = 0.8128$ ). Because there was no significant difference between modified and viable oocyst recoveries, average recoveries were used in all subsequent data analyses.

**Relation between *Cryptosporidium* recoveries and water quality characteristics.** The average recoveries obtained by

TABLE 4. *Cryptosporidium* recoveries in samples seeded with viable and modified oocysts

Stream water site	Stream flow condition	Viable oocysts					Modified oocysts			
		Vol filtered (liters)	Pellet vol (ml)	Vol examined (liters)	Adjusted oocyst recovery (%) <sup>a</sup>	IMS positive controls	Vol filtered (liters)	Pellet vol (ml)	Vol examined (liters)	Adjusted oocyst recovery (%) <sup>a</sup>
Alabama 1	Elevated	8.3	0.3	8.3	17	64	9.0	0.3	9.0	22
Alabama 2a	Elevated	8.3	0.1	8.3	37	77	8.5	0.1	8.5	59
Alabama 2b	Elevated	7.0	0.5	7.0	2.0	67	7.5	0.8	4.7	13
Colorado 1	Effluent	9.0	1.5	3.0	24	82	9.5	1.0	4.8	12
Colorado 2	Elevated	8.5	0.3	8.5	20	61	9.3	0.3	9.3	19
Georgia 1	Base	9.5	0.3	9.5	10	61	8.5	0.3	8.5	9.1
Georgia 1	High	5.0	0.5	5.0	10	67	5.0	0.5	5.0	13
Georgia 2	High	8.8	1.0	4.4	14	67	9.0	0.5	9.0	3.1
Indiana	Elevated	9.0	0.5	9.0	32	50 <sup>b</sup>	9.3	0.5	9.3	29
Iowa	Base	8.8	0.2	8.8	29	76	8.8	0.2	8.8	22
Iowa	High	9.8	1.0	4.9	2.0	74	9.8	1.0	4.9	4.0
Louisiana	Base	8.8	0.1	8.8	61	87	9.5	0.1	9.5	51
Louisiana	Elevated	8.0	0.5	8.0	23	76	9.0	0.5	9.0	20
Nebraska	High	3.0	0.7	2.1	2.8	61	5.0	1.5	1.6	3.0
Nebraska	Base	9.5	0.5	9.5	42	77	9.5	0.5	9.5	32
Ohio	Elevated	9.8	0.3	9.8	15	61	9.8	0.3	9.8	25
Ohio	High	9.8	0.5	9.8	40	82	9.3	0.5	9.3	51
South Carolina 1	Base	9.8	0.1	9.8	49	67	9.8	0.1	9.8	30
South Carolina 1	Elevated	10	0.3	10	32	58	10.5	0.3	10.5	28
South Carolina 2	Elevated	10	0.6	8.3	17	58	9.8	0.6	8.1	21
Texas	Elevated	7.5	0.8	4.7	18	87	8.2	1.0	4.1	12
Texas	Base	9.5	0.4	9.5	25	79	8.5	0.4	8.5	24
Virginia 1	Base	8.5	0.1	8.5	21	77	8.5	0.1	8.5	12
Virginia 2	Elevated	9.0	0.2	9.0	34	74	9.5	0.2	9.5	42
Washington 1a	Base	10	0.2	10	28	79	10	0.2	10	25
Washington 1b	Base	10	0.5	10	21	82	10	0.5	10	23
Washington 2	High	8.5	0.5	8.5	10	67	7.8	0.5	7.8	15
Wisconsin 1	High	8.5	2.5	1.7	15	61	9.5	2.5	1.9	20
Wisconsin 2	Base	9.0	0.9	5.0	27	79	8.8	0.8	6.5	37
Wisconsin 2	High	7.0	0.5	7.0	38	74	7.0	0.6	5.8	29
Avg		8.4	0.5	7.3	23.8	71.8	8.6	0.6	7.7	23.6

<sup>a</sup> If pellet volume was greater than 0.5 ml, the entire sample volume was not examined. Oocyst recovery was adjusted for the pellet volume examined.

<sup>b</sup> Slide was dropped and cracked, so counts are underestimated; this value was not used in average and statistical analyses.

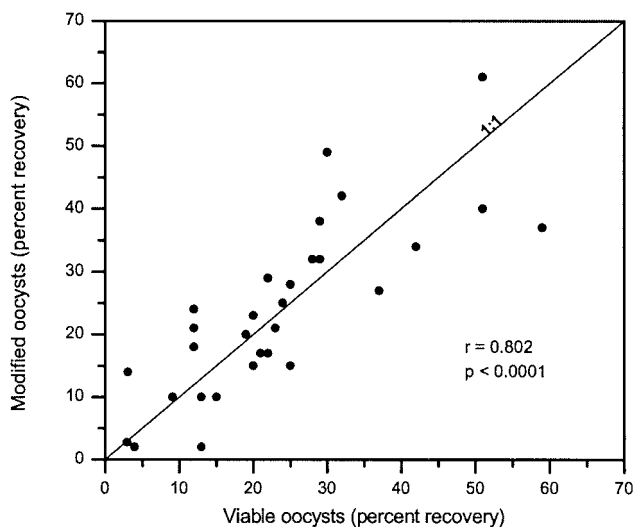


FIG. 1. Recoveries of viable oocysts (conventional seeding procedure) compared to recoveries of modified oocysts; r, Pearson's correlation coefficient; p, significance of the correlation.

using viable and modified oocysts were used to examine the relations between average recoveries and water quality properties and constituents (Table 5). Correlation analysis showed no significant relation ( $\alpha = 0.05$ ) between average recovery and pH, specific conductance, dissolved iron or silica, or alkalinity. Significant negative correlations were found between average oocyst recovery and turbidity or suspended sediment (Fig. 2). For samples with turbidities greater than 100 nephelometric turbidity units (NTU) and suspended-sediment concentrations greater than 100 mg/liter (Fig. 2, top of each graph), average recoveries were less than 20%. For samples with turbidities in the middle range (10 to 100 NTU), a wide range of average recoveries was found (8.6 to 56%); for those in the low range (<10 NTU), a slightly narrower range of average recoveries was found (17 to 48%). A similar pattern was seen in a comparison of average recoveries for suspended-sediment results.

At the 10 sites where two samples were collected, the percent differences in average recoveries between the two samples were calculated and ranged from 6 to 171% (Table 5). The three largest percent differences in recoveries (Alabama 2, Iowa, and Nebraska) were found for sample pairs that also had large differences in turbidities. The lowest percent difference (Wisconsin 2) was a sample pair collected at base and high

TABLE 5. Physical and chemical water quality analyses of stream water samples<sup>a</sup>

Stream water site	Stream flow condition	% Average recovery of modified and viable oocysts	% Difference in recoveries for samples from the same site	pH	Specific conductance (μS/cm)	Dissolved iron (mg/liter)	Dissolved silica (mg/liter)	Turbidity (NTU)	Suspended sediment (mg/liter)	Alkalinity (mg/liter)
Alabama 1	Elevated	20		7.8	165	<10	6.2	39	35	63
Alabama 2a	Elevated	48	146	8.0	86	25	4.5	1.4	2.6	24
Alabama 2b	Elevated	7.5		7.8	96	172	3.5	155	ND	39
Colorado 1	Effluent	18		6.5	3,850	384	15	26	ND	ND
Colorado 2	Elevated	20		8.1	1,380	24	10	9.8	14	189
Georgia 1	Base	9.6	22	7.1	186	107	8.4	14	17	31
Georgia 1	High	12		7.1	190	125	7.1	59	165	20
Georgia 2	High	8.6		7.1	80	70	8.2	95	202	21
Indiana	Elevated	31		8.0	662	684	7.6	34	ND	223
Iowa	Base	26	159	7.5	906	18	17	1.8	41	313
Iowa	High	3.0		8.0	751	<10	20	208	610	244
Louisiana	Base	56	87	7.8	467	72	17	17	82	149
Louisiana	Elevated	22		6.8	199	144	9.1	34	74	64
Nebraska	High	2.9	171	8.1	545	<10	14	2,700	778	232
Nebraska	Base	37		8.4	533	<10	15	9.1	13	205
Ohio	Elevated	20	79	7.8	736	ND	ND	1.8	98	ND
Ohio	High	46		8.1	632	8.0	7.3	15	63	234
South Carolina 1	Base	40	29	7.1	132	51	5.6	2.2	30	30
South Carolina 1	Elevated	30		6.3	108	143	7.5	5.1	7.0	21
South Carolina 2	Elevated	19		6.2	48	153	3.4	15	45	5.0
Texas	Elevated	15	50	7.8	447	7.0	4.0	101	287	126
Texas	Base	25		7.3	667	18	7.8	35	55	100
Virginia 1	Base	17		7.1	345	53	7.8	7.3	3.0	60
Virginia 2	Elevated	38		8.0	443	15	3.6	8.3	9.8	183
Washington 1a	Base	27	20	8.0	327	22	22	15	52	112
Washington 1b	Base	22		8.0	406	<10	30	73	28	136
Washington 2	High	13		7.3	72	85	6.4	28	108	24
Wisconsin 1	High	18		7.5	519	36	4.9	425	378	190
Wisconsin 2	Base	32	6	8.3	724	13	7.3	19	17	202
Wisconsin 2	High	34		7.8	714	ND	ND	15	ND	192

<sup>a</sup> ND, not determined.

flows with similar turbidities. Of the remaining six sample pairs in the intermediate group, all but two had higher recoveries in the sample with lower turbidity.

**Concentrations of *Cryptosporidium* oocysts and microbiological and chemical indicators.** Wide ranges of concentrations of *E. coli*, *C. perfringens*, somatic and F-specific coliphage, and chemical constituents associated with fecal contamination were found in the stream water samples (Table 6). The only sample in which *E. coli* was not detected was a high-flow sample from the Wisconsin 2 site, a mixed urban and agricultural area with the potential for contamination from septic systems, feedlots, manure, and wastewater treatment plants. *C. perfringens* and somatic coliphage were detected in all samples, and F-specific coliphage was detected in 72% of the samples. The highest concentrations of *C. perfringens* (Nebraska), somatic coliphage (Alabama 2), and F-specific coliphage (Washington 1) were found at three strictly agricultural sites. Two samples from Iowa had concentrations of nitrate above the maximum contaminant level for drinking water (10 mg/liter).

Five samples were positive for *Cryptosporidium*, two at elevated flow, two at base flow, and one from effluent (Table 6). Concentrations in the five positive samples, not adjusted for average recoveries, ranged from 1 to 6 oocysts/10 liters. When these concentrations were adjusted for average recoveries, they increased to a range of 4 to 80 oocysts/10 liters. Detection limits, adjusted for recoveries, ranged from <2 to <215 oocysts/10 liters. The five positive samples were in unseeded

samples; no endemic oocysts were found in any of the samples seeded with modified oocysts. Of the four positive stream water samples, three were from agricultural areas where animals were present (Alabama 1 and 2b and Washington 1) and one was from a mixed urban and agricultural area (Texas). Both Alabama sites were positive for *Cryptosporidium*; feedlots are upstream from Alabama 1, and free-range cattle have access to the stream at Alabama 2. The Texas site represents a large watershed, whereas the other positive sites are smaller watersheds (Table 1). The Alabama 1 site has the highest population density and the Washington 1 site has the lowest population density (Table 1) among the four stream water sites positive for *Cryptosporidium*. Because oocysts were found in a small percentage of samples (16.7%), the relations between detections of *Cryptosporidium* and concentrations of microbiological and chemical indicators could not be determined.

## DISCUSSION

Method 1623 is widely used to monitor source waters and drinking water supplies and is the required method in the proposed Long-Term 2 Enhanced Surface Water Treatment Rule (34). Therefore, modifications to reduce analytical costs and to improve recoveries are needed. In this study, a variety of stream water samples were collected from diverse geographical locations throughout the United States to test a new product, ColorSeed, to determine if it would yield results compa-

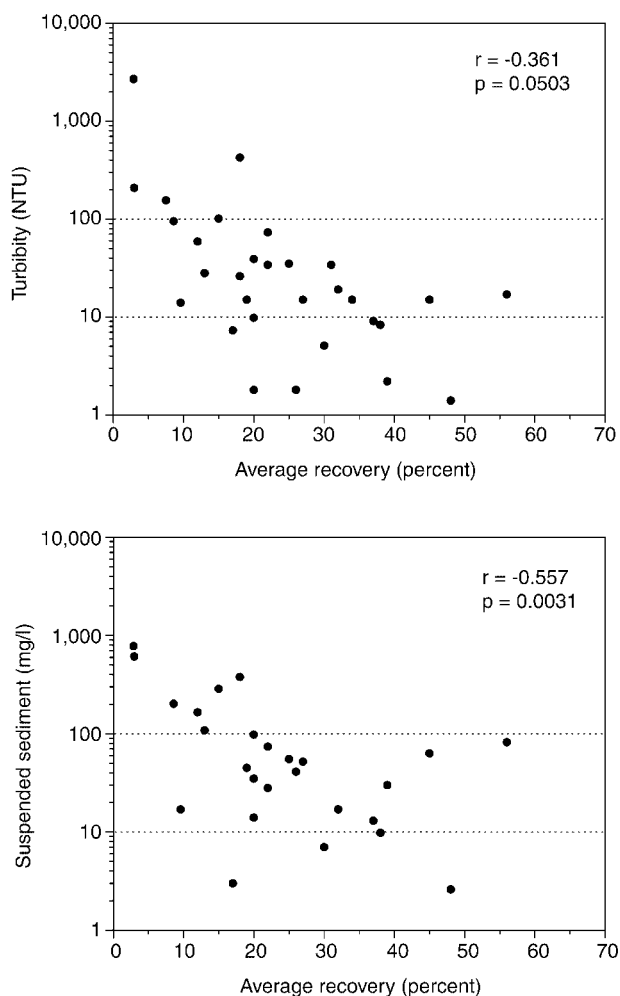


FIG. 2. Relations between average recoveries of oocysts (viable and modified) and water quality variables;  $r$ , Pearson's correlation coefficient;  $p$ , significance of the correlation.

able to those of conventional seeding procedures. This study also afforded the opportunity to collect data on the use of method 1623 for routine monitoring. We demonstrated the importance of including appropriate quality control samples in any monitoring program, examined the effects of water quality variables on method recovery efficiency of oocysts, and determined that the low percentage of environmental samples positive for *Cryptosporidium* precluded examining the relations between detections of oocysts and concentrations of potential microbiological or chemical indicators of fecally impacted waters.

Quality control samples provide insight into method efficiency and laboratory performance. IPRs, OPRs, and method blanks are required components of method 1623, whereas IMS controls are not required. Confirmation and trip control microscopic counts of oocysts to be used in matrix spikes are also not required components of method 1623. In this study, most IPRs and all OPRs were within acceptable limits and were comparable for viable and modified oocysts. IMS controls were always higher than IPR and OPR recoveries (except when

there was a laboratory error), indicating that oocysts were consistently lost during the filtration and concentration steps. The IMS controls indicated that the IMS reagents and process were working to the level expected. In examining confirmation and trip controls, microscopic counts were always less than certified counts of viable or modified oocysts. This observation could be due to oocyst degradation over time and during travel, the inability to transfer all the seed oocysts from their container to the sample, losses during other processing steps, or a failure to identify all oocysts on the slides by the analyst. Nevertheless, the differences showed minimal effects of travel and time on the condition of oocysts except when oocysts traveled through a four-legged trip (groups A and D). During analysis of environmental samples in this study, each set of samples traveled a three-legged trip (from USEPA to USGS to UNC).

As specified by method 1623, matrix spikes are required for every 20th sample or when a new water source is tested. We included a matrix spike for every sample analyzed. We found that, in some cases, recoveries were quite different between two samples collected at the same site, especially when turbidities were different. We also found that when average recoveries were considered in the calculations for some samples, concentrations of ambient oocysts increased considerably over those calculated without considering average recoveries. Determining recovery efficiency also provided data to calculate detection limits; in this study, a wide range of detection limits was found among sites and samples. It would appear prudent to collect and process matrix spikes not only when a new water source is tested but also when a sample is collected at a different stream flow or turbidity than previously collected and tested at a site.

During the course of this study, we found no statistically significant differences in recoveries when modified seeding procedures were used compared to recoveries when conventional seeding procedures were used. This finding is in contrast to a recently published Australian study of 247 raw water and 247 finished water samples in which recoveries were significantly lower for ColorSeed oocysts than for unmodified oocysts (36). The authors maintained, however, that the differences in recoveries were small, with mean value differences ranging from 3 to 5%, and concluded that ColorSeed is suitable for use as a control for routine monitoring (36). Our study supports this conclusion and showed that the use of modified oocysts was comparable to conventional seeding procedures. Unfortunately, we did not have the simultaneous occurrence of modified and environmental oocysts, so we could not evaluate the recognition of modified oocysts in a mixed sample.

In this study, average recoveries of oocysts (modified and viable) ranged from 2.9 to 56%. This wide range is similar to those found in other studies using method 1622 or 1623. In the analysis of 11 stream water samples, percent recoveries ranged from 2 to 63% (26). In the ICRSS, 65% of the 430 samples collected from 87 source waters had recoveries ranging from 20 to 60%, 13% had recoveries less than 20%, and 22% had recoveries greater than 60% (32). Kuhn and Oshima (15) analyzed 19 surface water sites and found that recoveries ranged from 9.3 to 87.7%.

For the environmental waters processed during this study, turbidity and suspended sediment were the only measured



TABLE 6. *Cryptosporidium* oocyst detections and concentrations of *E. coli*, *C. perfringens*, somatic and F-specific coliphage, and water quality constituents in stream water samples<sup>a</sup>

Stream water site	Stream flow condition	<i>Cryptosporidium</i>			<i>E. coli</i> (CFU/100 ml)	<i>C. perfringens</i> (CFU/100 ml)	Somatic coliphage (PFU/100 ml)	F-specific coliphage (PFU/100 ml)	Nitrite plus nitrate (mg/liter)	Total phosphorus (mg/liter)
		Oocysts (per 10 liters)	Vol examined (liters)	Estimated oocysts adjusted for avg recovery (per 10 liters)						
Alabama 1	Elevated	1	9.0	6	260	20	120	9	1.52	0.177
Alabama 2a	Elevated	0	8.0	<2	7	12	18	1	1.31	0.002
Alabama 2b	Elevated	6	5.0	80	1,800	250	>3,000	5	ND	ND
Colorado 1	Effluent	3	3.0	18	30	240	180	23	ND	ND
Colorado 2	Elevated	0	9.2	<6	19	150	440	35	7.02	0.910
Georgia 1	Base	0	8.3	<13	23	120	15	3	2.72	0.070
Georgia 1	High	0	5.0	<17	730	190	220	50	0.83	0.136
Georgia 2	High	0	5.3	<22	2,000	470	250	66	0.60	0.170
Indiana	Elevated	0	9.2	<4	110	67	74	<1	0.92	0.135
Iowa	Base	0	9.0	<4	11	20	46	<1	17.8	0.015
Iowa	High	0	5.0	<66	510	200	200	4	21.1	0.490
Louisiana	Base	0	9.5	<2	390	200	30	15	0.08	0.380
Louisiana	Elevated	0	7.5	<6	2,200	270	800	360	0.35	0.310
Nebraska	High	0	1.6	<215	18,000	900	1,400	29	3.37	1.09
Nebraska	Base	0	9.5	<3	7	70	17	<1	0.96	0.163
Ohio	Elevated	0	9.2	<5	200	30	260	10	4.10	0.080
Ohio	High	0	9.5	<2	210	80	150	3	4.57	0.061
South Carolina 1	Base	0	9.5	<3	140	45	150	84	2.19	0.010
South Carolina 1	Elevated	0	10.2	<3	180	150	270	<1	1.98	0.049
South Carolina 2	Elevated	0	8.3	<6	93	260	11	2	0.23	0.055
Texas	Elevated	0	4.0	<17	160	56	130	4	2.05	0.490
Texas	Base	2	8.5	10	2,700	100	31	6	8.43	1.94
Virginia 1	Base	0	8.8	<7	41	35	10	1	0.65	0.033
Virginia 2	Elevated	0	9.8	<3	12	22	480	<1	6.62	0.069
Washington 1a	Base	1	10	4	300	28	1,300	620	0.87	0.188
Washington 1b	Base	0	10	<4	170	90	24	<1	2.96	0.266
Washington 2	High	0	8.8	<9	770	400	94	5	0.43	0.156
Wisconsin 1	High	0	1.7	<33	13,000	190	2,800	<1	4.97	0.620
Wisconsin 2	Base	0	4.6	<7	100	120	16	5	<0.05	0.180
Wisconsin 2	High	0	6.2	<5	<1	200	100	<1	0.97	0.126
Median					180	120	140	4	1.75	0.160

<sup>a</sup> ND, not determined.

water quality characteristics that were significantly related to recoveries. An inverse relation was found for these characteristics and method efficiency, resulting in a decrease in recovery for high turbidities or suspended-sediment concentrations (>100 NTU or >100 mg/liter, respectively). These results are similar to those of other studies in which the effect of turbidity was investigated by adding known numbers of organisms to whole-water samples before the samples were processed by using method 1622 or 1623. Using a high-volume capsule filter, investigators found that recoveries of oocysts from source waters ranged from 36 to 75%; the lowest recovery was in the sample with the highest turbidity (99 NTU), and no relation between turbidity and recovery was found for samples with low to moderate turbidities (7). Kuhn and Oshima (15) found similar results with an analysis of 19 surface water samples. When turbidity was greater than 40 NTU, some decreases in recovery did occur; no relation was observed between oocyst recoveries and low or moderate turbidities (15). In this study, the effect of turbidity on recoveries was shown on a site-by-site basis at the 10 sites where we collected samples twice (Table 5). Of the 10 sample pairs, only 2 pairs behaved contrary to conventional wisdom (Georgia 1 and Ohio); that is, for these two samples, average recovery was higher when turbidity was

lower. This result demonstrates that one can generally expect lower recoveries with higher turbidities at the same sampling site.

In this study, initial water pH, specific conductance, dissolved iron, dissolved silica, and alkalinity did not affect recoveries of oocysts. Kuhn et al. (16) found that the IMS kit did not adequately maintain an optimum pH of 7.0 in some water samples. By adjusting the pH of concentrated water samples to optimum pH, recoveries of oocysts increased by 26.4% compared to recoveries from samples where pH was not adjusted (16). We did not evaluate the pH for the concentrated water sample prior to IMS but instead found that the initial sample pH and alkalinity did not affect recovery efficiency. Yakub and Stadterman-Knauer (38) found that dissolved iron concentrations greater than 4 mg/liter affected recoveries of oocysts; however, this concentration was greater than iron concentrations found in the course of our study (the highest dissolved iron concentration was 684 µg/liter) or in typical flowing surface waters (12). Similarly, silica concentrations in this study were typical of those in natural waters (1 to 30 mg/liter) (12) and did not affect recoveries of oocysts. In the ICRSS, total organic carbon concentrations, total suspended solids, temperature, dissolved organic carbon, bromide, ammonia, and

UV<sub>254</sub> did not affect method performance. Total dissolved solids, pH, specific conductance, and alkalinity weakly affected method performance (32).

Considerable effort was taken to collect samples in streams with potential sources of fecal contamination and under conditions with a greater potential for contamination of water samples. Nevertheless, *Cryptosporidium* oocysts were detected in only 16.7% of samples collected during this study and at low concentrations. In this study, concentrations ranged from 1 to 6 oocysts per 10 liters before adjustment for recoveries and 4 to 80 oocysts per 10 liters after adjustment for recoveries. Similar detection frequencies and lower concentrations were found in other recent source water studies wherein samples were analyzed by use of method 1622 or 1623. For the ICRSS, 12% of the source water samples were positive for oocysts (32). In a study of six source waters (17), *Cryptosporidium* oocysts were detected in 60 of 593 (10.1%) samples. Average concentrations, not adjusted for recoveries, ranged from <0.01 to 0.69 oocysts per 10 liters; the highest concentration was 10.17 oocysts per 10 liters (17).

In summary, variable recoveries of oocysts from the studied source waters suggest that water resource managers should consider increasing the frequency of the collection of matrix spikes. This is especially important when source water quality conditions change in response to increased stream flow. The use of a modified seeding procedure provided a reliable estimate of oocyst recoveries compared to the conventional seeding procedure and could be used to reduce the cost of additional matrix spikes. Turbidity and suspended-sediment concentrations affected oocyst recoveries, especially when turbidity was examined on a site-by-site basis.

#### ACKNOWLEDGMENTS

This research was funded by an Interagency Agreement between the U.S. Environmental Protection Agency Office of Research and Development and the U.S. Geological Survey.

Use of trade, product, or firm names is for descriptive purposes only and does not imply endorsement by the U.S. Government.

#### REFERENCES

1. Arrowood, M. J., and K. Donaldson. 1996. Improved purification methods for calf-derived *Cryptosporidium parvum* using discontinuous sucrose and cesium chloride gradients. *J. Eukaryot. Microbiol.* **43**:89S.
2. Atherholt, T. B., M. W. LeChevallier, W. D. Norton, J. J. Voorhees, and J. S. Rosen. 1998. Effect of rainfall on *Giardia* and *Cryptosporidium*. *J. Am. Water Works Assoc.* **90**:66–80.
3. Bonadonna, L., R. Briancesco, M. Ottaviani, and E. Veschetti. 2002. Occurrence of *Cryptosporidium* oocysts in sewage effluents and correlation with microbial, chemical, and physical water variables. *Environ. Monit. Assess.* **75**:241–252.
4. Bukhari, Z., R. M. McCuin, C. R. Fricker, and J. L. Clancy. 1998. Immunomagnetic separation of *Cryptosporidium parvum* from source water samples of various turbidities. *Appl. Environ. Microbiol.* **64**:4495–4499.
5. Campbell, A., and H. Smith. 1997. Immunomagnetic separation of *Cryptosporidium* oocysts from water samples: round robin comparison of techniques. *Water Sci. Technol.* **35**:397–401.
6. Cicmanec, J. L., and D. J. Reasoner. 1997. Enhanced production of *Cryptosporidium parvum* oocysts in immunosuppressed mice, p. 127–132. In C. R. Fricker, J. L. Clancy, and P. A. Rochelle (ed.), *Proceedings of the International Symposium on Waterborne Cryptosporidium*. American Water Works Association, Denver, Colo.
7. DiGiorgio, C. L., D. A. Gonzalez, and C. C. Huitt. 2002. *Cryptosporidium* and *Giardia* recoveries in natural waters by using Environmental Protection Agency method 1623. *Appl. Environ. Microbiol.* **68**:5952–5955.
8. Fishman, M. J. 1993. Methods of analysis by the U.S. Geological Survey National Water Quality Laboratory—determination of inorganic and organic constituents in water and fluvial sediments. U.S. Geological Survey open-file report 93–125. U.S. Geological Survey, U.S. Department of the Interior, Denver, Colo.
9. Fishman, M. J., and L. C. Friedman. 1989. Methods for determination of inorganic substances in water and fluvial sediments. U.S. Geological Survey TWRI 5A1. U.S. Geological Survey, U.S. Department of the Interior, Washington, D.C.
10. Guy, H. P. 1969. Laboratory theory and methods for sediment analysis. U.S. Geological Survey TWRI 5C1. U.S. Geological Survey, U.S. Department of the Interior, Washington, D.C.
11. Helsel, D. R., and R. M. Hirsch. 1992. *Statistical methods in water resources*. Elsevier Science Publishing Company, New York, N.Y.
12. Hem, J. D. 1989. Study and interpretation of the chemical characteristics of natural water, 3rd ed. U.S. Geological Survey water supply paper 2254. U. S. Geological Survey, U.S. Department of the Interior, Reston, Va.
13. Hirsch, R. M., W. M. Alley, and W. G. Wilber. 1988. Concepts for a national-water quality assessment program. U.S. Geological Survey circular 1021. U. S. Geological Survey, U.S. Department of the Interior, Reston, Va.
14. Kennedy, E. J. 1984. Discharge ratings at gaging stations. U.S. Geological Survey TWRI 3A10. U.S. Geological Survey, U.S. Department of the Interior, Washington, D.C.
15. Kuhn, R. C., and K. H. Oshima. 2002. Hollow-fiber ultrafiltration of *Cryptosporidium parvum* oocysts from a wide variety of 10-L surface water samples. *Can. J. Microbiol.* **48**:542–549.
16. Kuhn, R. C., C. M. Rock, and K. H. Oshima. 2002. Effects of pH and magnetic material on immunomagnetic separation of *Cryptosporidium* oocysts from concentrated water samples. *Appl. Environ. Microbiol.* **68**:2066–2070.
17. LeChevallier, M. W., G. D. Di Giovanni, J. L. Clancy, Z. Bukhari, S. Bukhari, J. S. Rosen, J. Sobrinho, and M. M. Frey. 2003. Comparison of method 1623 and cell culture-PCR for detection of *Cryptosporidium* spp. in source waters. *Appl. Environ. Microbiol.* **69**:971–979.
18. LeChevallier, M. W., W. D. Norton, and R. G. Lee. 1991. Occurrence of *Giardia* and *Cryptosporidium* spp. in surface water supplies. *Appl. Environ. Microbiol.* **57**:2610–2616.
19. Payment, P., A. Berte, M. Prevost, B. Menard, and B. Barbeau. 2000. Occurrence of pathogenic microorganisms in the Saint Lawrence River (Canada) and comparison of health risks for populations using it as their source of drinking water. *Can. J. Microbiol.* **46**:565–576.
20. Payment, P., and E. Franco. 1993. *Clostridium perfringens* and somatic coliphages as indicators of the efficiency of drinking water treatment for viruses and protozoan cysts. *Appl. Environ. Microbiol.* **59**:2418–2424.
21. Rose, J. B., H. Darbin, and C. P. Gerba. 1988. Correlations of the protozoa, *Cryptosporidium* and *Giardia*, with water quality variables in a watershed. *Water Sci. Technol.* **20**:271–276.
22. Rose, J. B., C. P. Gerba, and W. Jakubowski. 1991. Survey of potable water supplies for *Cryptosporidium* and *Giardia*. *Environ. Sci. Technol.* **25**:1393–1400.
23. Rouquet, V., F. Homer, J. M. Brignon, P. Bonne, and J. Cavard. 2000. Source and occurrence of *Giardia* and *Cryptosporidium* in Paris rivers. *Water Sci. Technol.* **41**:79–86.
24. Shelton, L. R. 1994. Field guide for collecting and processing stream-water samples for the National Water-Quality Assessment Program. U.S. Geological Survey open-file report 94–455. U. S. Geological Survey, U.S. Department of the Interior, Sacramento, Calif.
25. Simmons, O. D., III, M. D. Sobsey, C. D. Heaney, F. W. Schaefer III, and D. S. Francy. 2001. Concentration and detection of *Cryptosporidium* oocysts in surface water samples by method 1622 using ultrafiltration and capsule filtration. *Appl. Environ. Microbiol.* **67**:1123–1127.
26. Simmons, O. D., III, M. D. Sobsey, F. W. Schaefer III, D. S. Francy, R. A. Nally, and C. D. Heany. 2001. Evaluation of USEPA method 1622 for detection of *Cryptosporidium* oocysts in stream waters. *J. Am. Water Works Assoc.* **93**:78–87.
27. U.S. Bureau of the Census. 1991. Census of population and housing, 1990. Data Tech. Doc., Public Law 94–171. Census Bureau, Department of Commerce, Washington, D.C.
28. U.S. Environmental Protection Agency. 1985. Test method for *Escherichia coli* and enterococci in water by the membrane-filter procedure. U.S. Environmental Protection Agency publication no. 600/4–85/076. U.S. Environmental Protection Agency, Cincinnati, Ohio.
29. U. S. Environmental Protection Agency. 1996. EPA Information Collection Rule microbial laboratory manual. U.S. Environmental Protection Agency publication no. 600/R-95/178. U.S. Environmental Protection Agency, Washington, D.C.
30. U.S. Environmental Protection Agency. 2001. Method 1622—*Cryptosporidium* and *Giardia* in water by filtration/IMS/FA. U.S. Environmental Protection Agency publication no. 821/R-01–026. U.S. Environmental Protection Agency, Washington, D.C.
31. U.S. Environmental Protection Agency. 2001. Method 1623—*Cryptosporidium* and *Giardia* in water by filtration/IMS/FA. U.S. Environmental Protection Agency publication no. 821/R-01–025. U.S. Environmental Protection Agency, Washington, D.C.

32. **U.S. Environmental Protection Agency.** 2001. Implementation and results of the information collection rule supplemental surveys. U.S. Environmental Protection Agency publication no. 815-R-01-003. U.S. Environmental Protection Agency, Washington, D.C.
33. **U.S. Environmental Protection Agency.** 2001. Method 1602—male-specific and somatic coliphage in water by single agar layer (SAL) procedure. U.S. Environmental Protection Agency publication no. 821/R-01-029. U.S. Environmental Protection Agency, Washington, D.C.
34. **U. S. Environmental Protection Agency.** 2003. Source water monitoring guidance manual for public water systems for the Long Term 2 Enhanced Surface Water Treatment Rule (LT2 Rule). U.S. Environmental Protection Agency publication no. 815/D-03-005. U.S. Environmental Protection Agency, Washington, D.C.
35. **Ware, M. W., L. Wymer, H. Lindquist, and F. W. Schaefer III.** 2003. Evaluation of an alternative IMS dissociation procedure for use with method 1622—detection of *Cryptosporidium* in water. *J. Microbiol. Methods* **55**:575–583.
36. **Warnecke, M., C. Weir, and G. Vesey.** 2003. Evaluation of an internal positive control for *Cryptosporidium* and *Giardia* testing in water samples. *Lett. Appl. Microbiol.* **37**:244–248.
37. **Wilde, F. D., and D. B. Radtke.** 1998. National field manual for the collection of water-quality data—field measurements. U.S. Geological Survey TWRI 9A6. U.S. Geological Survey, U.S. Department of the Interior, Reston, Va.
38. **Yakub, G. P., and K. L. Stadterman-Knauer.** 2000. Evaluation of immunomagnetic separation for recovery of *Cryptosporidium parvum* and *Giardia duodenalis* from high-iron matrices. *Appl. Environ. Microbiol.* **66**:3628–3631.